

ACCUREF K-900/R-800

Auto Ref-Keratometer / Refractometer



About Us

Rex + Max = Rexam

Rexam, which means 'the king of the kings', is a respected and reliable brand.

Rexam is a Japanese company with a celebrated 60 year history. With over 3,000 employees worldwide, Rexam manufacture a wide range of products for various industries; from factory automation, automobiles and air conditioning systems, to beer and ski boots.

Since 1986, Rexam has manufactured various high quality products for leading brands in the eye care industry, including SHIN-NIPPON. Rexam had developed and manufactured products for SHIN-NIPPON since 1993 and in 2014 the company took over the SHIN-NIPPON brand.

We will be bringing high quality ophthalmic equipment to a global market. By combining precision engineering with industry leading innovation and experience in mass production, Rexam produce unique products to support eye care specialists across the world.

Quality in vision care, we are Rexam.



1960
Foundation of Rexam

1986
Rexam started the development and manufacturing of ophthalmic devices as an OEM supplier

1993
Rexam became the main OEM partner for SHIN-NIPPON
SHIN-NIPPON

2014
Rexam acquired the SHIN-NIPPON brand
SHIN-NIPPON by **Rexam**

2018
The manufacturer brand Rexam was inaugurated
Rexam

Rexam
Quality in vision care

Proudly  Made in Japan



Classic - Compact - Ergonomic Design

Rexxam's Auto Ref-Keratometer K-900 & Auto Refractometer R-800 offer accurate and reliable objective measurement results. This classic, compact, ergonomic design ensures easy and comfortable operation to eye-care professionals in their daily practices.


- Small footprint
- WTW measurement
- (Scotopic) Pupil measurement
- IOL mode
- Minimum pupil size $\Phi 2.0$ mm
- Connectivity with Digital Refractor DR-900
- Wide measurement range

Practical and comfortable to use




Monitor - Flexible Vertical-Horizontal Tilt Angle

Monitor 30° left-horizontal tilt allows the user to measure whilst supporting the patient. The 40° vertical tilt enables the user to operate comfortably at standing or sitting positions.

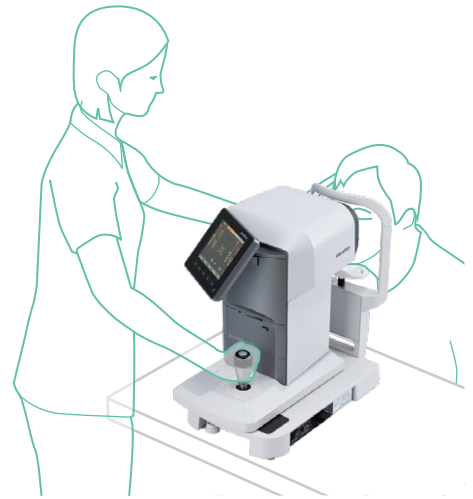


IOL Mode (Colour focus indicator)

Intraocular Lens (IOL) mode allows the possibility to measure eye with implanted Intraocular lens. The Red/Green focus indicator makes alignment easy, especially where irregular reflection occurs with some implanted IOL's.

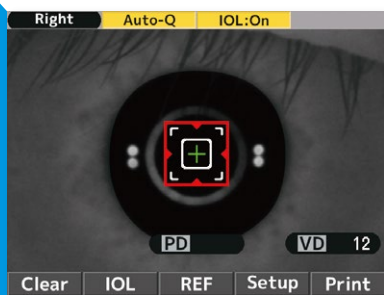

Color changes to green when focus is achieved

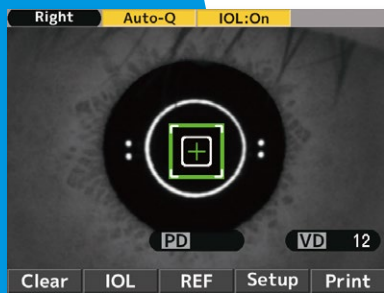

WTW measurement

WTW (White-to-White) corneal diameter measurement is an important factor for various ophthalmic applications such as contact lens fitting, etc.



Pupil diameter measurement

ACCUREF K-900 / R-800 have pupil size measurement functions. Pupil diameter is taken automatically during objective measurement and Scotopic Pupil Size (SPS) measurement can be taken without objective measurement.



Lateral headrest

The inward-curve design of the examination window section prevents strong light from directing to patient's eyes and minimises distraction. The headrest/chinrest sections keep the patient in comfortable position during measurement.



Capacitive touch sensor buttons

The capacitive touch sensor buttons work responsively whilst keeping the main screen clear from fingerprints, etc.



Intuitive joystick operation

The Joystick is solid and ergonomically built to ensure maximum comfort and intuitive fast operation.



Comprehensive print out

- Selective Printout in 3 different formats:
- Up to 10x REF data + KRT data
- Up to 10x REF data + KRT data (average)
- Only average REF data + KRT data

Breath shield

A dedicated breath-shield is available as an option in case of social distancing requirements. (Optional)



When all setting items are enabled

| | | |
|--|------------------------|-----------------------------|
| , ABCDEFGH I JKLMNOPQRSTU VWX , abcdefgh i jklmnopqrstuvw x | | Message Area |
| No. 00001 | | |
| NAME 2011 11 22 14:30 | | Date & Time |
| VD=12 | | |
| IOL Mark | <R> SPH CYL AX PPS | Photopic Pupil Diameter |
| | 1 - 3.87 -0.75 172 5.4 | Ref Value |
| Reliability Warning Indicator | 1 - 3.87 -0.75 170 5.3 | |
| | 1 - 3.87 -0.62 174 5.4 | |
| Scotopic Pupil Diameter | SPS 7.3 | Ref Representative Value |
| <R> mm D AX | | Kerato Value |
| R1 | 8.43 40.00 9 | |
| R2 | 8.21 41.12 99 | |
| AVE | 8.32 40.62 9 | |
| CYL | -1.12 9 | |
| R1 | 8.43 40.00 10 | |
| R2 | 8.22 41.12 100 | |
| AVE | 8.32 40.50 10 | |
| CYL | -1.12 10 | |
| R1 | 8.30 40.62 2 | |
| R2 | 8.16 41.37 92 | |
| AVE | 8.23 41.00 92 | |
| CYL | -0.75 2 | |
| R1 8.31 40.62 180 | | Kerato Representative Value |
| R2 8.17 41.37 90 | | |
| AVE 8.24 41.00 90 | | |
| CYL -0.75 180 | | |
| Residual Astigmatism | REST -0.21 131 | |
| <L> SPH CYL AX PPS | | Left Eye |
| - 3.75 -1.12 13 6.6 | | |
| - 3.75 -1.12 15 6.6 | | |
| - 3.75 -1.12 14 6.6 | | |
| - 3.75 -1.12 14 6.6 | | |
| SPS 6.9 | | |
| Near PD | PD = 65 NPD = 62 (50) | |
| Far PD | | |
| Rexxam ACCUREF K-900 | | |
| Interpupillary Measurement Function | | |



| | | | K-900 | R-800 |
|--|---|------------------------------------|---|-------|
| Refractive Measurement Range (Ref Measurement) | Sphere (S) | Measurement Range | -30D ~ +22D (VD=12) -22D ~ +30D (VD=0) | |
| | | Step | 0.12D, 0.25D (Switching) | |
| | Cylinder (C) | Measurement Range | 0D ~ ±10D (VD=0) | |
| | | Step | 0.12D, 0.25D (Switching) | |
| | | Symbol | -, +, ± (Switching) | |
| | Axis (A) | Measurement Range | 0° ~ 180° | |
| | | Step | 1°, 5° | |
| Vertex Distance | | 0, 10, 12, 13.5, 15 mm | | |
| Minimum Pupil Diameter Measurable | | Φ2.0 mm | | |
| Corneal Curvature Radius Measurement | Corneal Curvature Radius | Measurement Range | 5.0 mm~ 10.0 mm | - |
| | | Step | 0.01 mm | - |
| | Corneal Refractivity | Measurement Range | 33.75D ~ 67.5D (where corneal refractive index n = 1.3375) | - |
| | | Step | 0.12D , 0.25D (Switching) | - |
| | Degree Of Corneal Astigmatism | Measurement Range | 0D ~ ±10D | - |
| | | Step | 0.12D , 0.25D (Switching) | - |
| | | Symbol | mm , -D , +D (Switching) | - |
| | Axis Angle | Measurement Range | 0° ~ 180° | - |
| Step | | 1° , 5° | - | |
| PD Measurement | Measurement Range | 85mm | | |
| | Step | 1mm | | |
| Pupil Diameter Measurement | Measurement Range | Φ2.0 mm ~ Φ8.5 mm | | |
| | Step | 0.1mm | | |
| Measurement Time | Refractive Measurement Range | approx. 0.07 sec. | | |
| | Corneal Curvature Radius Measurement | approx. 0.07 sec. | - | |
| Fog Contrl | Fogging for Each Measurement (Auto) Fogging is Provided at the First Measurement Followed by Continuous Measurement (Auto-Quick) | | | |
| Monitor | 5.7 inch color LCD monitor | | | |
| Printer | Thermal line printer | | | |
| Power | Power Voltage | AC 100 ~ 240 V , 50/60Hz | | |
| | Power Consumption | 60VA | | |
| | Power Saving Function | OFF , 3 , 5 , 10 min. (selectable) | | |
| Data Output | R2-232C interface | | | |
| Size | Weight | approx. 13kg | | |
| | Dimensions | 240mm(W) × 422mm(D) × 430mm(H) | | |
| Movement Range of The Measurement Unit | Forward - Backward : ±22mm Right - Left : ±43mm Up - Down : ±17mm | | | |
| Movement Range of The Chin Rest | Up - Down : ±30mm | | | |
| Movement Range of LCD | Swivel : left 30° Vertical Tilt : up 40° | | | |

Standard Accessories

- Model Eye
- Printer Roll Paper
- Chin Rest Paper
- Chin Rest Paper Pin
- Spare Fuse
- Dust Cover

Design and specifications are subject to change without prior notice.

Manufacturer

Rexxam
Quality in vision care

Rexxam Co.,Ltd.
Kagawa factory

958 Ikeuchi, Konan-cho,
Takamatsu-shi, Kagawa-ken,
761-1494 Japan

Contact

Rexxam Co.,Ltd.
Eye-care Instruments Sales Dept. Tokyo Office

2-4-2 Kandatsukasa-machi, Chiyoda-ku, Tokyo,
101-0048 Japan
TEL:+81-3-6262-9471 FAX:+81-3-6262-9472
E-mail:eye@rexexam.co.jp
Website:https://www.rexxam.co.jp

Distributed by

Proudly Made in Japan

Rexxam



/ Rexxam



LinkedIn

